
Quick Guide



Cardio Q70 & Q50

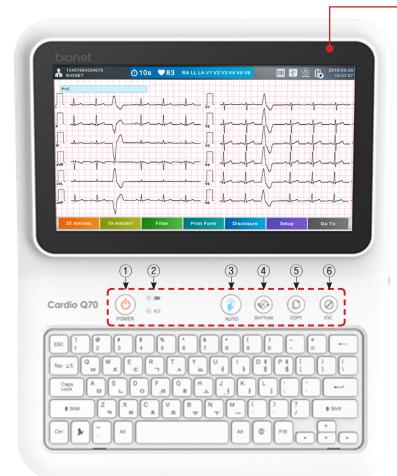

LCD Touchscreen

- Cardio Q70 : 10.1"
- Cardio Q50:8"

Front View

1 POWER

② LED Indicator: Power connection / Battery status

3 AUTO

Short Press: Start the AUTO workflow from ECG data acquisition, transmission, and printing out ECG diagnosis with one single operation

Press & Hold for 3 sec: 10 sec ECG data acquisition and printing out in the selected format


- (4) **RHYTHM**: Print out ECG waveform in real-time or in a report size
- (5) COPY: Print out the selected data after processing the ECG data in the same or modified form
- (6) **ESC**: Cancel the operation command and return to the previous mode of the main menu

Back View



- **(1) AC Power Connection Port**
- **(2)** Protective Ground Terminal
- (3) USB Port (2ea)
- (4) HDMI Port
- **(5) RJ45 LAN Port**

Right Side View

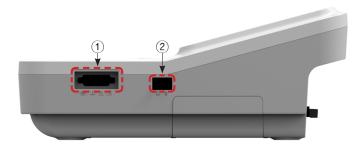

1 Patient Cable Connection Port

2 USB Port (Spiro Handle Port)

Quick Guide Cardio Q70 & Q50

1. Power On

Press and hold the power button.

2. Login

Input proper ID and password and press the LOGIN button.



3. Worklist / Patient Registration

Opt 1. Press Worklist \rightarrow Find the patient in the list.

Opt 2. Press ECG \rightarrow Press [No Patient] to register the patient info.

Opt 3. Connect a barcode reader and scan the patient barcode.

		QWO	orklist 🔣 🚺	1/9 🕨			💷 🛿 🖧 🖏	2019-01
Cardio	Q70	1	05082710	takdq	м	43yr	2019-05-08 11:07:30	ECG
		2	05082710	takdq	м	43yr	2019-05-08 11:07:19	SVC
		з	05082710	takdq	м	43yr	2019-05-08 11:07:16	MVV
		4	05082710	takdq	м	43yr	2019-05-08 11:07:04	FVC
		5	05082705	swamb		64yr	2019-05-08 11:06:02	ECG
Worklist ECG	Spiro File	6	05082704	tdviw	м	54yr	2019-05-08 11:05:56	ECG
Worklist ECG	Spiro File	7	05082703	whivj	м	32yr	2019-05-08 11:05:49	ECG
		8	05082702	utrhe	м	46yr	2019-05-08 11:05:45	ECG
		9	05082701	pdovj	м	42yr	2019-05-08 11:05:39	ECG
Copyright @ Bionet Co	o., Ltd.	So	lect Exem	Update Patient			Setup G	o To

No Patient	0 10:	s 🎔 60	RA LL LA V1 V2 V	3 V4 V5 V6) 🛄 🛿 🖧	2019-05- 10:22:
Л		l-	~"I _	~		
I -dr			~v_	~ ~~~		
l	-44-	~h	~u -	-fr-nf	ndp	-fr-
	p		~	-ll	n	-h-
"l <u> </u>		·^		~~~~	\	
		~	~	~~~~	n	
25 mm/sec	10 mm/mV	Filter	Print Form	Disclosure	Setup	Go To

4. Locate Electrodes

Touch [Lead Fault Information Indicator] located in the middle of upper menu bar of ECG main screen, the image will show to indicate the location for attaching the leads.

No Patient	<mark>()</mark> 10s	♥60	RA LL LA VI V2 V	3 V4 V5 V6	•	II 🛛 🖧	2019-05-08
-							
	hh-		~,i	-	~~~	-fr-	
	handha		~v	-fr-	f	-h-	-fr
l	bb-	~^	~	h	h	m	-fr
ve ^l	pp-		~~~~ , l -	-h-	-h-	-h-	
"l	<u> </u>			-	-h-	h	
,	hh-		~∬	-h	-		
	and all	Filler	Dyint Farm	Distant		Catur	



6. Preview

You can check the automatic analysis result on the preview screen.

7. OK

Press OK to finish the AUTO key procedures.

Proview anotae Vasu 9	Heat Bale Khan Photo an Interaction Of Data (Heat Mark and Data) Photo and Data (Heat Sciences 4 Alt (Heat)	4.0heant + Hillythin Report ** Anglesis Read ** (Erich Kindy confirmed to confidency) Named Read Theory Named Read Symmet 10:01	Personal and a second sec
internet	- Ar		
-	-		hh
		- A A B	hand
			hand
1 I			h
-h-h			
int	- In the	- h- h- h-	-the the
Bentime UP Hite ACKing DAGON		Zeneri week	
25 mm/sec 10 m	nm/mV Filter	Print Form Patient	Ok Cancel

5. AUTO

Press the AUTO button to acquire data for 10 seconds.



You can set the AUTO key function at the Setup \rightarrow File \rightarrow Auto menu.

8. Check the exam data

You can check the exam data in the **Patient** menu or the **File** menu.

Headquarters Bionet Co., Ltd.

5F, 61 Digital-ro 31gil, Guro-gu, Seoul 08375, REPUBLIC OF KOREA TEL. +82 2 6292 6410 E-mail. sales@ebionet.com www.ebionet.com